




Nasal or saliva sample and buffer are added to the test well. Any SARS-CoV-2 antigens contained in the sample will start to flow down the strip.

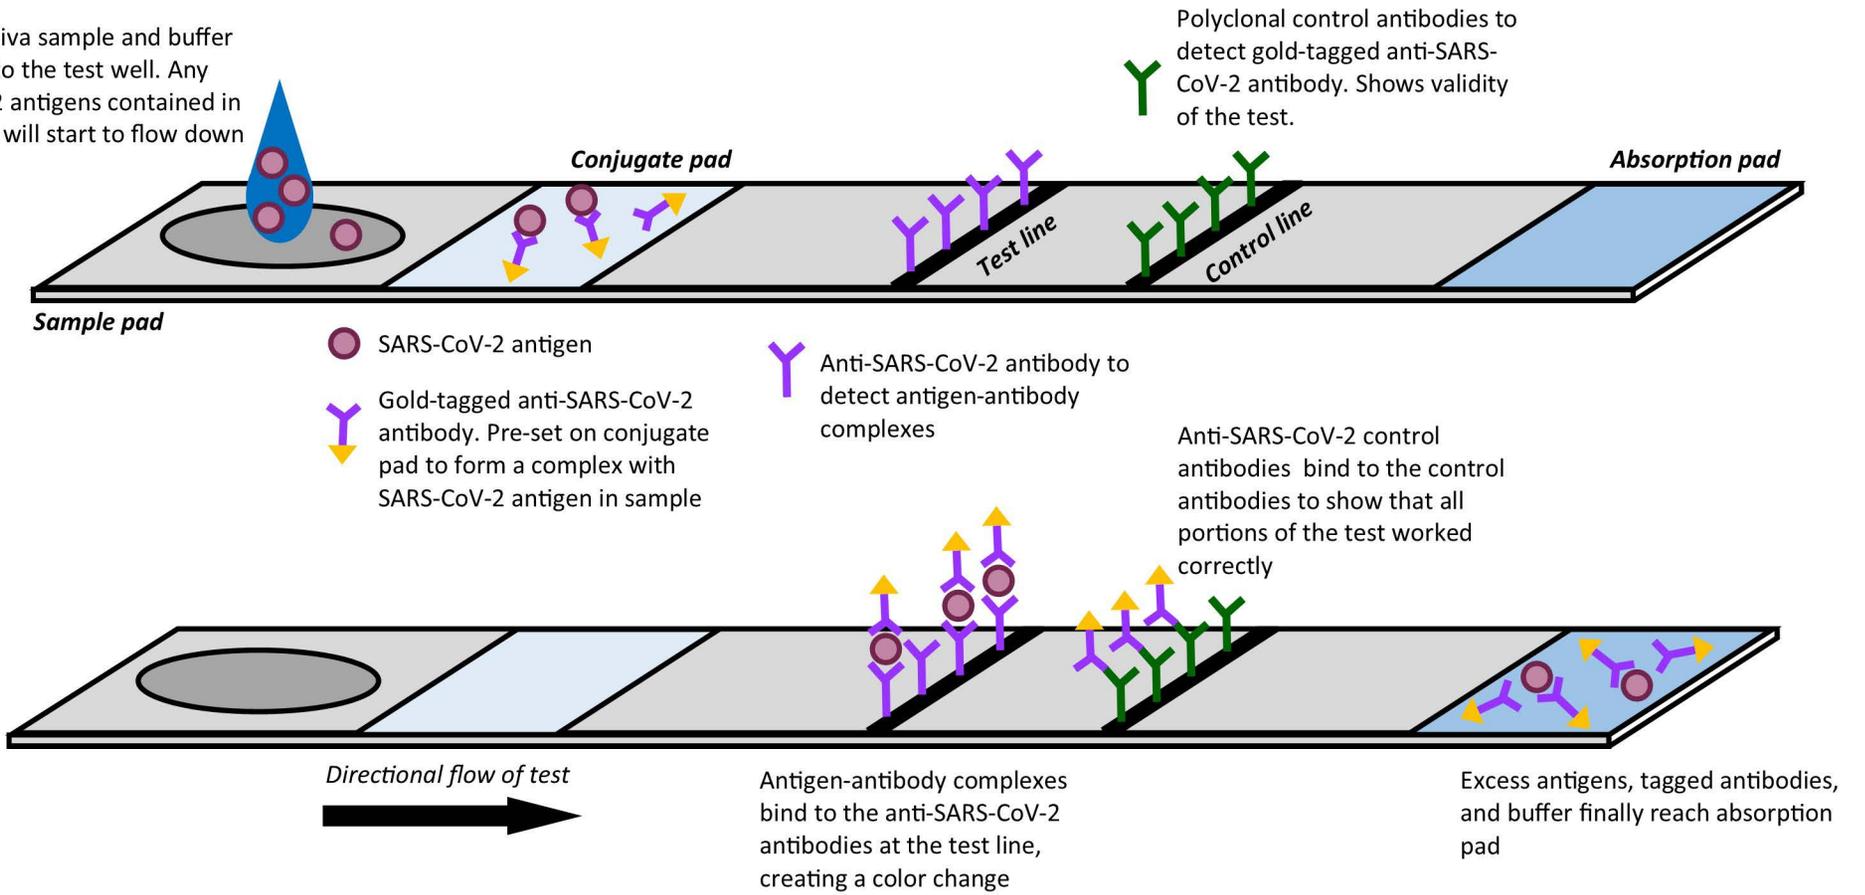


Positive Result

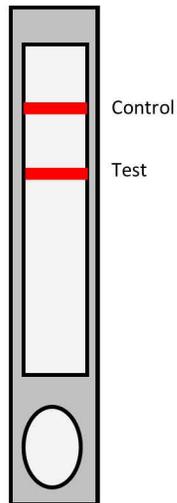

Negative Result

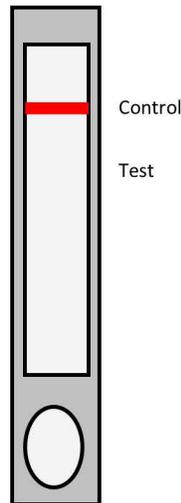

Inconclusive Result

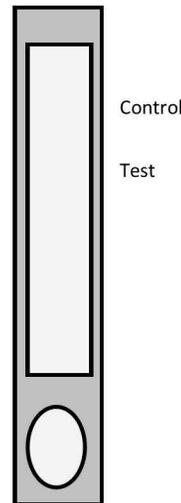

Inconclusive Result

